

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 1 of 18		REVISION G
	AUTHORIZED BY S ALOSIOUS		DATE 10 JUN 14
		STATUS UNRESTRICTED	

TABLE OF CONTENTS

1.0	OBJECTIVE.....	3
2.0	SCOPE	3
3.0	GENERAL	3
3.1.	Usage.....	3
3.2.	Visual	3
3.3.	Banded Substances.....	3
3.4.	Manufacturing Processability.....	3
4.0	APPLICABLE DOCUMENTS	4
4.1.	Standards and Specifications	4
4.2.	FCI Documents	4
4.2.1.	Process Specifications	4
4.2.2.	Standards and Test Specifications	5
4.3.	Lab Reports - Supporting Data	5
5.0	REQUIREMENTS.....	5
5.1.	Qualification	5
5.2.	Material	5
5.2.1.	Metallic Parts.....	5
5.2.2.	Plastic Parts	6
5.3.	Finish	6
6.0	ELECTRICAL CHARACTERISTICS	6
6.1.	Low Level Contact Resistance	6
6.2.	Insulation Resistance.....	7
6.3.	Dielectric Withstanding Voltage	7
6.4.	Current Rating.....	7
6.5.	Capacitance	7
6.6.	Inductance	8
6.7.	Propagation Delay	8
6.8.	Characteristic Impedance	8
6.9.	Crosstalk	9
7.0	MECHANICAL CHARACTERISTICS.....	10
7.1.	Mating/Unmating Force	10
7.2.	Header Signal Compliant Pin Insertion/Retention Force.....	10
7.3.	Receptacle Signal Compliant Contact Insertion/Retention Force	10
7.4.	PCB Hole Deformation Radius	10
7.5.	PCB Hole Wall Damage	10

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row		PAGE 2 of 18	REVISION G
		AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14
		STATUS UNRESTRICTED	

8.0	ENVIRONMENTAL CONDITIONS.....	11
8.1.	Thermal Shock.....	11
8.2.	Humidity	11
8.3.	High Temperature Life	11
8.4.	Mixed Flowing Gas (4-Gas).....	12
8.5.	Vibration Sinusoidal	12
8.6.	Mechanical Shock.....	12
8.7.	Durability	12
8.8.	Dust Contamination	13
8.9.	Disturb.....	13
9.0	QUALITY ASSURANCE PROVISIONS.....	13
9.1.	Equipment Calibration	13
9.2.	Inspection Conditions	13
9.3.	Sample Quantity and Description	13
9.4.	Acceptance	13
9.5.	Qualification Testing	13
9.6.	Re-Qualification Testing	14
9.7.	Qualification Test Sequence Per Table 1	14
9.8.	Qualification Test Sequence Per Table 2	16

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 3 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
	STATUS UNRESTRICTED		

1.0 **OBJECTIVE**

This specification defines the performance, test, quality, reliability and signal integrity requirements of 8 row Metral™ Standard, 1000 & 2000 family of products.

Standard product

74771-type 8 Row Metral™ Standard Header
 98173-type 8 Row Metral™ Standard Shroud
 74770-type 8 Row Metral™ Standard Receptacle
 74983-type 8 Row Metral™ 1000 Header
 74978-type 8 Row Metral™ 2000 Header
 74993-type 8 Row Metral™ 1000 Shroud
 84625-type 8 Row Metral™ 2000 Shroud
 74981-type 8 Row Metral™ 1000 Receptacle
 10041744-type 8 Row Metral™ 1000 Receptacle

Selectively Loaded Product

84965-type 8x12 Metral™ Standard Header
 98030-type 8x12 Metral™ Standard Header
 63784-type 8x12 Metral™ 1000 Header
 63741-type 8x12 Metral™ 2000 Header
 84964-type 8x12 Metral™ 1000 Receptacle

2.0 **SCOPE**

This specification is applicable to the termination characteristics of the Metral™ Standard, 1000 & 2000 family of products. Metral™ Standard, 1000 & 2000 products provide a board-to-board matched impedance interconnect.

3.0 **GENERAL**

3.1. Usage

The headers, shrouds and receptacles covered by this instruction are intended for use in a wide variety of environments.

3.2. Visual


Visual examinations shall be performed with a magnification up to 10X (8 to 10X recommended). Parts should be free from blistering, cracks, discoloration, etc.

3.3. Banned/Restricted Substances

All product where the part number ends in 'LF' meet the European Union directives and other country regulations as described in GS-22-008. The part numbers that do not end in 'LF' meet all regulations except for Pb in SnPb plating.

3.4. Manufacturing Processability

All products covered by this specification will withstand exposure to 260°C for 60 seconds in a convection, infra-red or vapor phase reflow oven.

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 4 of 18		REVISION G
	AUTHORIZED BY S ALOSIOUS		DATE 10 JUN 14
	STATUS UNRESTRICTED		

4.0 **APPLICABLE DOCUMENTS**

The following documents, of issue in effect at the date of latest revision of this specification, shall form a part of this specification to the extent specified herein.

4.1. **Standards and Specifications**

ASTM B488: Electrodeposited Coatings of the Au /GXT for Engineering Uses

UL94V-0: Tests for Flammability of Plastic Materials in Devices and Appliances

IEC 512: International Electrical Commission Standards

IEC 61076-4-104: Connectors For Use In DC, Low Frequency Analogue And Digital High Speed Data Applications

GR-1089-CORE: Telcordia Specification “Electromagnetic Compatibility and Electrical Safety - Generic Criteria for Network Telecommunications Equipment”


GR-1217-CORE, Issue 1, November 1995: Telcordia Specification “ Generic Requirements for Separable Electrical Connectors”

EIA-364: Electrical Connector/Socket Test Procedures Including Environmental Classifications

4.2. **FCI Documents**

4.2.1. **Process Specifications**

Specification	Description
BUS-01-040	VG Site Equipment Calibration Guidelines
BUS-15-002/X	Nickel Plating
BUS-15-006/X	Tin/Lead Plating
BUS-15-008	Palladium Nickel Alloy Plating
BUS-15-005/X	The Au /GXT in Contact Plating
GS-46-001	Tin (lead free) Plating
BUS-19-020	Porosity, Plating
BUS-19-040	Adhesion, Plating

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 5 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
	STATUS UNRESTRICTED		

4.2.2. Standards and Test Specifications

Specification	Description
BUS-03-108	Qualification Lab Method and Procedure-Crosstalk Test Methods
BUS-03-110	Qualification Lab Method and Procedure-Characteristic Impedance
BUS-03-111	Qualification Lab Method and Procedure-Propagation Delay Measurements
BUS-03-113	Qualification Lab Method and Procedure-Induction Measurements
BUS-03-114	Qualification Lab Method and Procedure-Capacitance Measurements
BUS-03-404	Normal Force Measurements
BUS-03-601	Current Rating / 30°C Temperature Rise

4.3. Lab Reports - Supporting Data

Supporting Data	EL 1997-10-082	EL 1998-010-039	EL 1999-02-091
	EL 1998-02-087	EL 1997-011-012	EL 2000-02-012B
	EL 2001-04-032	EL 2001-07-049	EL 2001-03-074
	EL 2001-03-074D	EL 1999-10-055 STD	EL 2001-08-019
	EL 2001-08-019A	EL 2001-02-025A	

5.0 REQUIREMENTS


5.1. Qualification

Connectors furnished under this specification shall be capable of meeting the qualification test requirements specified herein.

5.2. Material

5.2.1. Metallic Parts

Contact, Receptacle: Copper Alloy Strip
 Top Shield, Receptacle: Copper Alloy Strip
 Vertical Shield, Receptacle: Copper Alloy Strip
 Bottom Shield, Receptacle: Copper Alloy Strip
 Pin, Header: Copper Alloy Strip
 Ground Spring, Header and Shroud: Copper Alloy Strip
 Stripline Shield, Header and Shroud: Copper Alloy Strip

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 6 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
	STATUS UNRESTRICTED		

5.2.2. Plastic Parts

Housing, Receptacle: LCP, GFR, Flame retardant UL94V-0, Natural
 IMLA, Receptacle: LCP, GFR, Flame retardant UL94V-0, Natural
 Housing, Header: LCP, GFR, Flame retardant UL94V-0, Natural
 Housing, Shroud: LCP, GFR, Flame retardant UL94V-0, Natural

5.3. Finish

Plated finishes for qualification components shall be as specified herein or equivalent. The receptacle contacts and header pins shall be qualified to the minimum thickness of either Au or GXT™ specified on product prints over a 1.3 µm minimum Ni underplate. The Au /GXT deposit shall meet the requirements of ASTM B488. Plating in press-fit area shall be Sn (lead free) over Ni if part number ends in 'LF' and SnPb over Ni if part number does not end in 'LF'.

Vertical receptacle shields shall be plated with 0.5 µm minimum Sn (lead free) over 1.2 µm minimum Ni if the part number ends in 'LF' and 0.5 µm minimum SnPb over 1.2 µm minimum Ni if the part number does not end in 'LF'. Top and bottom receptacle shields shall be plated with a minimum The Au /GXT plating thickness specified on product prints over a 1.3 µm minimum Ni underplate. Plating in press-fit area shall be Sn (lead free) over Ni if part number ends in 'LF' and SnPb over Ni if part number does not end in 'LF'.

Header and shroud ground springs shall be plated with a 1.3 µm minimum Ni followed by the minimum The Au /GXT plating thickness specified on product prints in the mating area. Plating in press-fit area shall be Sn (lead free) if part number ends in 'LF' and SnPb if part number does not end in 'LF'.


Header stripline shields shall be plated with Sn (lead free) over 1.3 µm Ni if the part number ends in 'LF' and SnPb over 1.3 µm Ni if the part number does not end in 'LF'. Shroud stripline shields shall be plated with a 1.3 µm minimum Ni followed by the minimum The Au /GXT plating thickness specified on product prints in pin connection areas. Shroud stripline shields shall be plated with Sn (lead free) over 1.3 µm Ni if the part number ends in 'LF' and SnPb over 1.3 µm Ni if the part number does not end in 'LF' in the ground spring mating areas.

6.0 ELECTRICAL CHARACTERISTICS

6.1. Low Level Contact Resistance

Measurements shall be performed using a four wire method with a maximum open circuit voltage of 20 mV and a maximum test current of 100 mA (see EIA-364-23). Maximum initial signal contact resistance is 12 mΩ. Initial to final measurements after environmental exposure shall not exceed a 10 mΩ change. Top, middle and bottom ground shields shall have an initial maximum contact resistance of 15 mΩ and also shall not exceed a 10 mΩ change.

- Test Voltage - 20 mV DC maximum open circuit
- Test Current - Not to exceed 100 mA

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row		PAGE 7 of 18	REVISION G
		AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14
		STATUS UNRESTRICTED	

6.2. **Insulation Resistance**

The insulation resistance of mated connector pair connectors shall not be less than 1000 MΩ after environmental exposure when measured in accordance with EIA-364-21. The following details shall apply:

- a) Test Voltage - 500 VDC
- b) Electrification Time - 1 minute
- c) Points of Measurement - Between adjacent contacts and between contacts and metal shields

6.3. **Dielectric Withstanding Voltage**

There shall be no evidence of arc-over, insulation breakdown or excessive leakage current (> 0.5 mA) when the mated connectors are tested in accordance with EIA-364-20. The following details shall apply:

- a) Test Voltage - 500 VDC or 500 VAC peak RMS or AC, 60 Hz.
- b) Test Duration - 60 seconds.
- c) Test Condition – 1 atm
- d) Voltage: Applied at a rate of 500 V per second.
- e) Points of Measurement - Between adjacent contacts and between contacts and the metal shields

6.4. **Current Rating**

The temperature rise above ambient shall not exceed 30°C at any point in the system when all contacts are powered at 1 A or one contact is powered at 3 A. The following details shall apply:


- a) Ambient Conditions - Still air at 25°C.
- b) Reference - BUS-03-601.

6.5. **Capacitance**

Note: The requirements listed below apply only to the Metral™ 1000 and 2000 connector systems. Requirements for the Metral™ Standard connector system will be published at a later date.

The specification requirement shall be satisfied when evaluated in accordance with FCI Test Specification BUS-03-114 and the following details:

- a) Specification requirement 3.0 pF max.
- b) Sample documentation
- c) Sample test conditions
 - Frequency: 1MHz
 - Amplitude: 1 V
 - Surrounding contacts tied to ground

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 8 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
	STATUS UNRESTRICTED		

6.6. Inductance

The specification requirement shall be satisfied when evaluated in accordance with FCI Test Specification BUS-03-113 and the following details:

- a) Specification requirement 15 nH max.
- b) Sample documentation
- c) Sample test conditions - 1 MHz

6.7. Propagation Delay

The specification requirement shall be satisfied when evaluated in accordance with FCI Test Specification BUS-03-111 and the following details:


- a) Specification requirement 300 pico-seconds max, 40 pico-seconds risetime 10 - 90% measured at 50%.
- b) Skew between adjacent rows not to exceed 40 pico-seconds, total skew not to exceed 150 pico-seconds.
- c) Sample documentation.

6.8. Characteristic Impedance

Note: The requirements listed below apply only to the Metral™ 1000 and 2000 connector systems. Requirements for the Metral™ Standard connector system will be published at a later date.

The specification requirement shall be satisfied when evaluated in accordance with FCI Test Specification BUS-03-110 and the details listed below. Note that one top shield j-hook (per connector) shifted to either side of the vertical shield constitutes acceptable workmanship and does not affect connector characteristic impedance.

- a) Specification requirement $55 \pm 5 \Omega$ single-ended except where Column 12 is not bounded by the shield of a neighboring module. In this case, the unshielded end column shall have a requirement of $61 \pm 5 \Omega$ single-ended.
- b) Sample documentation.
- c) Sample test conditions @ 500 pico-seconds (10 - 90%) risetime with all lines terminated in its characteristic impedance.

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 9 of 18		REVISION G
	AUTHORIZED BY S ALOSIOUS		DATE 10 JUN 14
	STATUS UNRESTRICTED		


6.9. Crosstalk


Note: The requirements listed below apply only to the Metral™ 1000 and 2000 connector systems. Requirements for the Metral™ Standard connector system will be published at a later date.

The specification requirement shall be satisfied when evaluated in accordance with FCI Test Specification BUS-03-108 and the details listed below. Note that one top shield j-hook (per connector) shifted to either side of the vertical shield constitutes acceptable workmanship and does not affect connector crosstalk.

- Specification requirement, less than 12% single active NEXT.
- Sample documentation.
- Sample test conditions, 500 pico-seconds rise time with all lines terminated in its characteristic impedance.

Figure 1 Crosstalk Test Setup

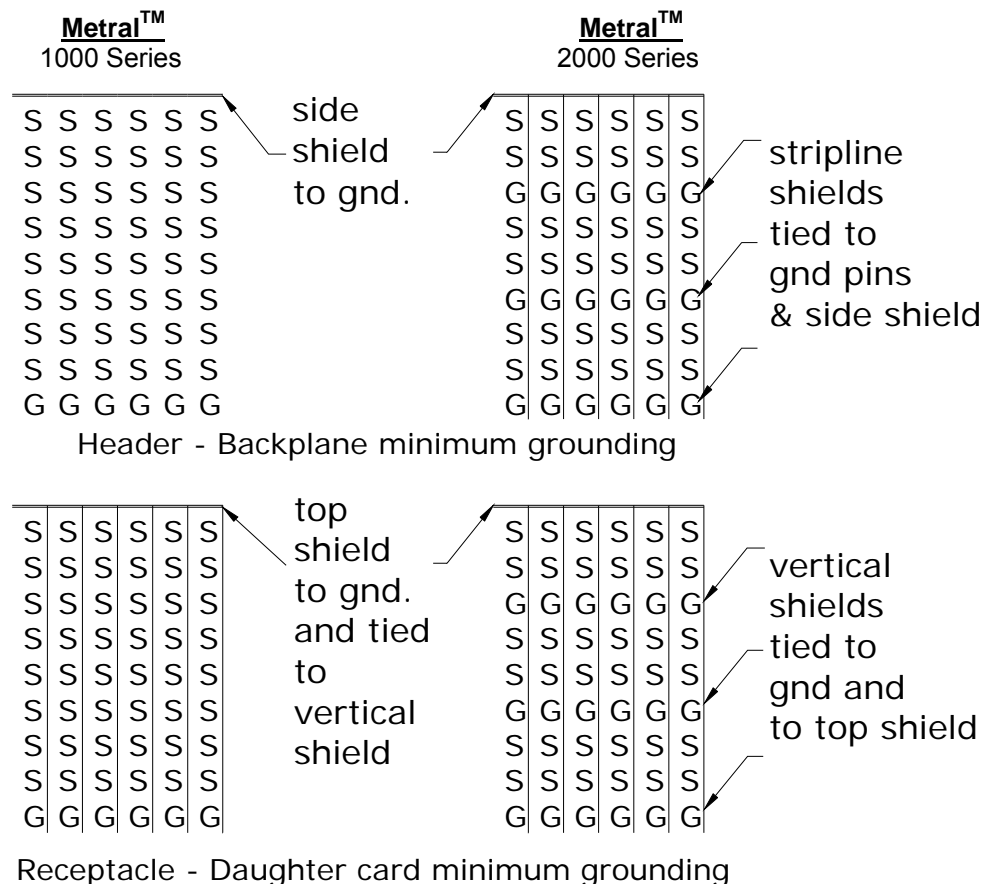

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 10 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
	STATUS UNRESTRICTED		

7.0 MECHANICAL CHARACTERISTICS

7.1. ***Mating/Unmating Force***

The force to mate a receptacle connector and compatible header shall not exceed 0.55 N per contact. The unmating force shall not be less than 0.15 N per contact. The following details shall apply:

- a) Cross Head Speed – 25.4 mm/minute (1 inch/minute).
- b) Lubrication - None
- c) Utilize free floating fixtures.
- d) Reference - EIA-364-13.

Total single module (8x12) mating force shall not exceed 62.7 N and total unmating force shall not be less than 17.1 N.

7.2. ***Header Signal Compliant Pin Insertion/Retention Force***

The force required to insert an individual signal compliant pin into a plated through hole in a printed circuit board at a rate of 5.1 mm/minute (0.2 inches/minute) shall not exceed 100 N. The retention force in an axial direction opposite that of insertion shall not be less than 20 N.

Total single module (8x12) insertion force shall not exceed 11,400 N when inserted by a standard application press.

7.3. ***Receptacle Signal Compliant Contact Insertion/Retention Force***

The force required to insert an individual signal compliant contact into a plated through hole in a printed circuit board at a rate of 5.1 mm/minute (0.2 inches/minute) shall not exceed 32 N. The retention force in an axial direction opposite that of insertion shall not be less than 7 N.


Total single module (8x12) insertion force shall not exceed 3776 N when inserted by a standard application press.

7.4. ***PCB Hole Deformation Radius***

Cross-section parallel to board surface. Photograph and measure the hole deformation (deformation of board material) radius at a point 0.25 mm (0.010 in) from the surface and at the center of the compliant pin section. The average hole deformation radius of 10 holes shall be no greater than 37.5 µm (0.0015 in) when measured from the finished hole. The absolute maximum deformation radius shall not exceed 50 µm (0.002 in). Reference Telcordia GR-1217-CORE, Section 5.1.7.

7.5. ***PCB Hole Wall Damage***

Cross-section perpendicular to the board surface and through the compliant section wear track. Photograph and measure the copper thickness remaining between the compliant pin and the printed wiring board laminate. The minimum average copper thickness of 10 holes remaining between the compliant pin and the printed wiring board laminate shall not be less than 7.5 µm (0.0003 in). In addition, there shall be no copper cracks, separations between conductive interfaces or laminate-to-copper separations. Reference Telcordia GR-1217-CORE, Section 5.1.7.

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 11 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
	STATUS UNRESTRICTED		

8.0 ENVIRONMENTAL CONDITIONS

After exposure to the following environmental conditions as specified in “**Table 1 - Test Sequences**” in accordance with the specified test procedure and/or details, the product shall show no physical damage and shall meet the electrical and mechanical requirements in Sections 6. and 7. Unless specified otherwise, product shall be mated during exposure.

8.1. Thermal Shock

EIA-364-32, Test Condition II

Test:

1. Number of cycles: 5
2. Temperature Range: Between -65°C +0°C/-5°C and +105°C +3°C/-5°C.
3. Time at each temperature: 30 minutes
4. Transfer time: 5 minutes maximum.

8.2. Humidity

Mated samples are to be exposed to cyclical humidity and temperature in accordance with EIA-364-31, Method IV, with the following exceptions. Samples are to be subjected to 50 cycles of 10 hour durations for a total of 500 hours (after 24 hours in a conditioning oven at 50±2°C). A cycle consists of the following steps.

Test:


1. Ramp from 25±2°C at 80%-98% RH to 65±2°C at 94±4% RH in 120 minutes.
2. Dwell at 65±2°C at 94±4% RH for 4 hours.
3. Ramp down to 25±2°C at 80%-98% RH in 120 minutes.
4. Dwell at 25±2°C at 80%-98% RH for 2 hours.

8.3. High Temperature Life

EIA-364-17, Method A, Test Condition 4. Headers and receptacles shall remain mated w/o any electrical load.

Test :

1. Temperature: 105±2°C
2. Duration: 1000 hours

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 12 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
	STATUS UNRESTRICTED		

8.4. **Mixed Flowing Gas (4-Gas)**

Samples are to be exposed to an industrial gas mixture in accordance with Telcordia GR-1217-CORE, Section 9.1.3. The headers ONLY are to be exposed for 10 days to the gas mixture detailed below, with interim resistance measurements made after the 5th and 10th days. The samples are then mated with the appropriate receptacle and exposed to an additional 10 days with resistance measurements taken after the 15th and 20th days of exposure. The test chamber is to be maintained at a temperature of 30±1°C with a relative humidity of 70±2%.

Per Central Office Requirement	
<u>Gas</u>	<u>Gas Concentration</u>
NO ₂	200 ppb
Cl ₂	10 ppb
H ₂ S	10 ppb
SO ₂	100 ppb

8.5. **Vibration Sinusoidal**

Perform in accordance with Telcordia GR-1217-CORE, Sections 6.3.5 and 9.1.2.1.

Test:

1. Vibration amplitude: 0.06 inch DA or 10G acceleration.
2. Frequency range: 10 to 500 Hz
3. Duration: 8 hours along each of three orthogonal axes
4. Mounting: Rigidly mounted assemblies
5. Requirement: No discontinuities greater than 10 nano-seconds for signal contacts, 1 micro-second for ground connections.

8.6. **Mechanical Shock**

Perform in accordance with Telcordia GR-1217-CORE, Sections 6.3.5 and 9.1.2.1.

Test:


1. Conditions: half-sine 30G, 11 milli-second duration.
2. Shocks: 3 shocks along each of three orthogonal axis.
3. Mounting: Rigidly mounted assemblies.
4. Requirement: No discontinuities greater than 10 nano-seconds for signal contacts, 1 micro-second for ground connections.

8.7. **Durability**

Standard laboratory procedure as applicable to the specific product.

Test:

1. Number of cycles: 98 or 99 cycles per “**Table 1 - Test Sequences**”.
2. Cycling rate: 127 mm/minute (5 inches/minute)
3. Mating and unmating forces to be measured per Section 7.1. on the first and last cycle.

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row		PAGE 13 of 18	REVISION G
		AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14
		STATUS UNRESTRICTED	

8.8. **Dust Contamination**

Perform in accordance with Telcordia GR-1217-CORE, Section 9.1.1.1 & Table 9-1 unmated.

8.9. **Disturb**

An Instron compression/tensile tester shall be used to back the fully seated receptacle from the header by 0.10 mm (0.004 in). The sample is then removed and measurements made.

9.0 **QUALITY ASSURANCE PROVISIONS**

9.1. **Equipment Calibration**

All test equipment and inspection facilities used in the performance of any test shall be maintained in a calibration system in accordance with ISO 9000.

9.2. **Inspection Conditions**

Unless otherwise specified herein, all inspections shall be performed under the following conditions:

Temperature: 25± 5°C

Relative humidity: 30% to 60%

Barometric pressure: Local ambient

9.3. **Sample Quantity and Description**

The test sequence for the qualification testing of the receptacle and header and sample size are shown in Tables 1 and 2. The minimum connections to be tested are specified in the descriptions of each test.


9.4. **Acceptance**

Electrical and mechanical requirements placed on test samples as indicated in the sections of this specification shall be established from test data using appropriate statistical techniques or shall otherwise be customer specified, and all samples tested in accordance with the product specification shall meet the stated requirements.

Failures attributed to equipment, test set-up or operator error shall not disqualify the product. If product failure occurs, corrective action shall be taken and samples resubmitted for qualification.

9.5. **Qualification Testing**

Qualification testing shall be performed on sample units with equipment and procedures normally used in production. The test sequence is shown in Tables 1 and 2.

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 14 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
	STATUS UNRESTRICTED		

9.6. Re-Qualification Testing

If any of the following conditions occur, the responsible product engineer shall initiate re-qualification testing consisting of all applicable parts of the qualification test matrix, Tables 1 and 2.

- a) A significant design change is made to the existing product, which impacts the product form, fit or function. Examples of significant changes shall include, but not be limited to, changes in the plating, material composition or thickness, contact force, pin/contact surface geometry, insulator or housing design, pin/contact base material or pin/contact lubrication.
- b) A significant change is made to the manufacturing process which impacts the product form, fit or function.
- c) A significant event occurs during production or end use requiring corrective action to be taken relative to the product design or manufacturing process

9.7. Qualification Test Sequence Per Table 1

The following connection points are to be tested for low level contact resistance in Test Groups 1 to 4 per Section 6.1 when called for in Table 1. When possible, resistance measurements should include the press-fit sections of the header and receptacle as well as the separable connection. Visual examination before any testing should confirm that the sample is not damaged or missing features. Visual examination after testing should confirm that the sample has not been damaged during testing except for the effects of the testing itself. All resistance measurements that are outside the limits should be confirmed before additional testing to assure that the measurements are correct.

TYPE OF CONNECTION	MIN. SAMPLE SIZE
Hdr. Signal Pin to Recept. Contact	100
Hdr. Ground Spring to Recept. Top Shield	96
Hdr. Ground Pin to Recept. Bottom Shield	100

For best results, use Metral™ 1000 headers for Test Groups 1 – 4 listed in Table 1. The Metral™ 2000 headers have stripline shields, which ground and common some of the pins to each other and the ground spring. For Test Groups 1 – 4, the minimum quantity can be reduced proportionally if monoblock parts are used.



	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 15 of 18		REVISION G
	AUTHORIZED BY S ALOSIOUS		DATE 10 JUN 14
	STATUS UNRESTRICTED		

Table 1 - Test Matrix

		TEST GROUP								
		1	2	3	4	5	6	7	8	9
MIN QUANTITY OF 8x12 REC		20	16	20	16	7	4	4	16	3
MIN QUANTITY OF 8x12 HEADERS		20	16	20	16	4	4	4	16	4
TEST	PARA	TEST SEQUENCE								
		MFG	Hi-Temp Life	Thermal Shock & Humidity	Vibration & Mech. Shock	PCB Hole Deform.	Elect. Perform.	Current Rating	Mating/Umating Force	EON Forces
EXAMINATION OF PRODUCT	3.2	1,22	1,6	1,16	1,14	1,5	1,7	1,3	1,3	1,5
MATE HEADER & RECEPTACLE		2,8,12	2	2,11	2,7					
UNMATE HEADER AND RECEPTACLE		6,10		9	5					
<u>ELECTRICAL CHARACTERISTICS</u>										
LOW LEVEL CONTACT RESISTANCE ¹	6.1	3,5,9,13,15,17,19,21	3,5	3,5,13	3,8,10,13					
INSULATION RESISTANCE ¹	6.2			6,14						
DIELECTRIC WITHSTANDING VOLTAGE ¹	6.3			7,15						
CURRENT RATING	6.4							2		
CAPACITANCE	6.5						2			
INDUCTANCE	6.6						3			
PROPAGATION DELAY	6.7						4			
CHARACTERISTIC IMPEDANCE	6.8						5			
CROSSTALK	6.9						6			
<u>MECHANICAL CHARACTERISTICS</u>										
MATING/UNMATING FORCE – 3 CYLCES	7.1								2	
COMPLIANT CONTACT										
INSERTION/RETENTION FORCE	7.2 & 7.3					2				2,4
PCB HOLE DEFORMATION RADIUS	7.4					3				
PCB HOLE WALL DAMAGE	7.5					4				
<u>ENVIRONMENTAL CONDITIONS</u>										
THERMAL SHOCK	8.1			4						
HUMIDITY	8.2			12						
HIGH TEMPERATURE LIFE	8.3		4							3
MFG HEADER ONLY (4-GAS) 5-DAYS	8.4	7,11								
MFG MATED (4-GAS) 5-DAYS	8.4	14,16								
VIBRATION SINUSOIDAL – 1 EACH AXIS	8.5				9					
MECHANICAL SHOCK	8.6				12					
DURABILITY 98 CYCLES	8.7	20								
DURABILITY 99 CYCLES	8.7	4		8	4,11					
DUST CONTAMINATION	8.8			10	6					
DISTURB	8.9	18								

1. Insulation resistance, dielectric withstanding voltage and low level contact resistance are to be measured on different contacts.

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
		PAGE 16 of 18	REVISION G
		AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14
		STATUS UNRESTRICTED	

TITLE	Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row
-------	---

9.8. Qualification Test Sequence Per Table 2


The following connections points are to be tested for low level contact resistance in Test Groups 10 to 17 per Section 6.1 when called for in Table 2. When possible, resistance measurements should exclude the press-fit sections of the header. Visual examination before any testing should confirm that the sample is not damaged or missing features. Visual examination after testing should confirm that the sample has not been damaged during testing except for the effects of the testing itself. All resistance measurements that are outside the limits should be confirmed before additional testing to assure that the measurements are correct.

TYPE OF CONNECTION	MIN. SAMPLE SIZE
Stripline Shield to Pin	100
Stripline Shield to Ground Spring	96

The testing per Table 2 checks the internal ground connections in the Metral™ 2000 headers and shrouds. When both headers and shrouds are being tested, the stripline shield-to-ground spring resistance changes need only be tested on either the header or shroud. The ground spring connection points are exactly the same design. For testing shrouds, a Metral 1000 rear plug-up (RPU) header must be inserted with the ground spring removed in the bottom side of the test board. The shroud is then assembled on the top side.


Table 2 - Test Matrix

		TEST GROUP							
		10	11	12	13	14	15	16	17
MIN QUANTITY OF 8x12 SHROUDS						16	16	16	16
MIN QUANTITY OF 8x12 HEADERS		16	16	16	16				
TEST	PARA	TEST SEQUENCE							
		MFG	Hi-Temp Life	Thermal Shock & Humidity	Vibration & Mech. Shock	MFG	Hi-Temp Life	Thermal Shock & Humidity	Vibration & Mech. Shock
EXAMINATION OF PRODUCT	3.2	1,11	1,5	1,8	1,11	1,11	1,5	1,8	1,11
<u>ELECTRICAL CHARACTERISTICS</u>									
LOW LEVEL CONTACT RESISTANCE	6.1	2,4,6,8,10	2,4	2,4,7	2,4,8,10	2,4,6,8,10	2,4	2,4,7	2,4,8,10
<u>ENVIRONMENTAL CONDITIONS</u>									
THERMAL SHOCK	8.1			3				3	
HUMIDITY	8.2			6				6	
HIGH TEMPERATURE LIFE	8.3		3				3		
MIXED FLOWING GAS (4-GAS) 5-DAYS	8.4	3,5,7,9				3,5,7,9			
VIBRATION SINUSOIDAL 1-EACH AXIS	8.5				5,6,7				5,6,7
MECHANICAL SHOCK	8.6				9				9
DUST CONTAMINATION	8.8			5	3			5	3

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 17 of 18		REVISION G
	AUTHORIZED BY S ALOSIOUS		DATE 10 JUN 14
	STATUS UNRESTRICTED		

REVISION RECORD

REV	PAGE	DESCRIPTION	EC #	DATE
A	ALL	NEW DOCUMENT	V02082	08/29/00
B	7	CHANGE TEMP. RANGE FOR HUMIDITY SEC. 8.2	V10853	02/06/01
C	ALL	•REVISE FORMAT	V20115	01/18/02
	5	•ADD NOTE – SEC 6.5		
	6	•SKEW BETWEEN ROWS 35 ps TO 40 ps / TOTAL SKEW 100 ps TO 150 ps -- SEC 6.7.b		
	6	•ADD NOTE -- SEC 6.8 & 6.9		
	7	•ADD TOTAL MATING FORCE / MIN UNMATING FORCE 0.20 N TO 0.17 N -- SEC 7.1		
	8	•ADD TOTAL INSERTION FORCE -- SECS 7.3 & 7.4		
	10	•ADD GROUND CONNECTION DISCONTINUITY REQUIREMENT -- SEC 8.5		
	13	•REMOVE DWV / ADD DISTURB -- TEST GROUP 1 TABLE 1		
	13	•REMOVE NORMAL FORCE & LLCR BETWEEN VIBRATION AXES -- TEST GROUP 4 TABLE 1		
	13	•REMOVE RISE TIME DEGRADATION -- TEST GROUP 6 TABLE 1		
	13	•ADD TEST GROUP 8 TABLE 1		
	13	•ADD METRAL™ 2000 HEADER & SHROUD INTERNAL		
	14	GROUND TESTING & TABLE 2 – SEC 9.8		
D	1,2	•MOVE TABLE OF CONTENTS TO BEGINNING	V20975	05/24/02
	4	•REMOVE MIL STDS – WAS SEC 4.1		
		•REMOVE US FEDERAL SPECS – WAS SEC 4.2		
	5	•ADD ASTM B488 – SEC 4.1		
		•ADD EL 2001-08-019, EL 2001-08-019A & EL 2001-02-025A – SEC 4.3		
		•CHANGE METALLIC DESIGNATIONS TO 'COPPER ALLOY' – SEC 5.2.1		
	8	•ADD SHIFTED J-HOOK NOTE - SECS 6.8 & 6.9		
	9	•MIN UNMATING FORCE 0.17 N TO 0.15 N & TOTAL UNMATING FORCE 19.4 N TO 17.1 N – SEC 7.1		
	10	•REMOVE CONTACT NORMAL FORCE REQUIREMENT – WAS SEC 7.2		
		•ADD 'SIGNAL' TO FORCE REQUIREMENTS – SECS 7.2 & 7.3		
		•CHANGE REFERENCE SPEC TO TELCORDIA GR-1217-CORE – SECS 7.4 & 7.5		
	12	•ADD TELCORDIA SECTION REFS 6.3.5 AND 9.1.2.1 – SEC 8.5		
		•REPLACE NOTE 4 RESISTANCE MEASUREMENTS WITH DISCONTINUITY REQUIREMENT – SEC 8.6		
		•REMOVE NORMAL FORCE – TEST GROUP 2 TABLE 1		
	15	•REVISE TEST SEQUENCE & RECEPTACLE TEST QUANTITY – TEST GROUP 5 TABLE 1		
		•ADD TEST GROUP 9 TABLE 1		
E	All	ADD LEAD FREE INFORMATION	V05-0879	09/14/05
F	All	Change logo	V06-0405	04/26/06

	TYPE PRODUCT SPECIFICATION	NUMBER GS-12-134	
TITLE Metral™ Standard Series – 8 Row Metral™ 1000 Series – 8 Row Metral™ 2000 Series – 8 Row	PAGE 18 of 18	REVISION G	
	AUTHORIZED BY S ALOSIOUS	DATE 10 JUN 14	
		STATUS UNRESTRICTED	

G	4 & 6	<ul style="list-style-type: none"> MODIFIED THE TEXT "AU" TO "AU /GXT" 	ELX-I-17965	11/06/14
	15 & 16	<ul style="list-style-type: none"> REMOVE THE TEXT "WITH 0.8 µm GOLD PLATING" 		
	6	<ul style="list-style-type: none"> MODIFIED THE TEXT "0,8um minimum thickness " TO "minimum thickness of either Au or GXT™ " 		
	ALL PAGES	<ul style="list-style-type: none"> AUTHORIZED & DATE CHANGED 		

Mouser Electronics

Authorized Distributor

Click to View Pricing, Inventory, Delivery & Lifecycle Information:

FCI:

[74978-102001](#) [74983-102011](#) [74983-102001LF](#) [74978-102011LF](#) [74770-102](#) [74978-102006](#) [74978-102051](#)
[74978-502011](#) [74983-102004](#) [74983-102050](#) [74983-102051](#) [74983-102054](#) [74983-502001](#) [74983-502011](#) [74978-](#)
[102011](#) [84625-102](#) [74978-102001LF](#) [10041744-102LF](#) [74978-102012LF](#) [74978-102013LF](#) [74978-102050LF](#) [74978-](#)
[102053LF](#) [74978-102054LF](#) [74983-102052LF](#) [74983-102058LF](#) [74983-502004LF](#) [74983-502061LF](#) [84964-102LF](#)
[74770-102LF](#) [74978-102006LF](#) [74978-102051LF](#) [74978-502011LF](#) [74983-102004LF](#) [74983-102011LF](#) [74983-](#)
[102050LF](#) [74983-102051LF](#) [74983-102054LF](#) [74983-502001LF](#) [74983-502011LF](#) [74993-102LF](#) [84625-102LF](#)
[74983-102001](#) [74978-102012](#) [74978-102013](#) [74978-102050](#) [74978-102053](#) [74978-102054](#) [74983-102013LF](#)
[74983-102052](#) [74983-102058](#) [74983-502004](#) [74983-502061](#) [74993-502](#) [84964-113](#) [84964-113LF](#) [74993-502LF](#)